




Knee Immobilizer

Single Patient Use Only

Rx Only

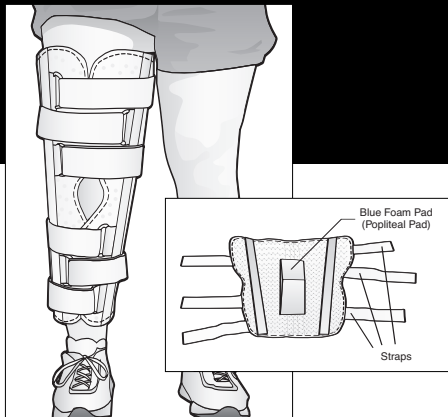

IMPORTANT INFORMATION

Please read carefully and completely before applying.

INTENDED USE

For immobilization of the knee joint, post-operatively or after joint injury.

INDICATIONS

Post-operative knee immobilization, Grade II or III ligament sprains.

CONTRAINDICATIONS

Patients with poor peripheral circulation, diabetes or decrease in skin sensitivity should not use a knee immobilizer.

PRECAUTIONS

- Consult your medical professional immediately if you experience sensation changes, unusual reactions, swelling or prolonged pain while using this product.
- The knee immobilizer should fit, generally, 2" above ankle bones and 2" below groin. Any longer could result in abnormal wear and skin pressure.

Sized Knee Immobilizer SIZING CHART







	Knee Circumference
S	14"-16"
M	16"-18"
L	18"-20"
XL	20"-22"
XXL	22"-24"
XXXL	24"-26"

INSTRUCTIONS FOR USE

- Place brace against the leg such that the metal stay runs down the back of the leg (anteriorly).
- If the blue foam popliteal pad is ordered by clinician, remove paper backing to expose adhesive and apply to the knee immobilizer as shown.
- Close the brace so that the patella notch surrounds the knee.
- Buckle the straps immediately below and above the knee joint. Buckle in an alternating below and above fashion until all of the straps are secure.
- Adjust all straps for a snug, yet comfortable fit.

CLEANING INSTRUCTIONS


Hand wash with mild detergent in lukewarm water.
Air dry.

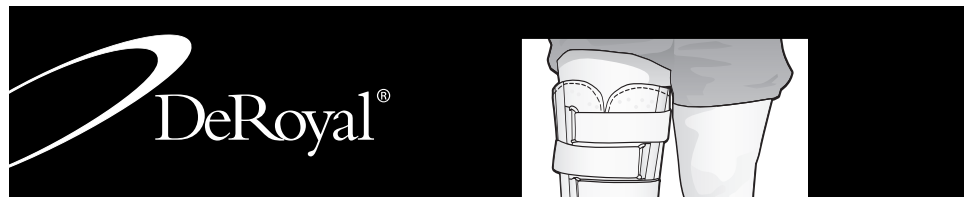

Knee Immobilizer

Single Patient Use Only

Rx Only

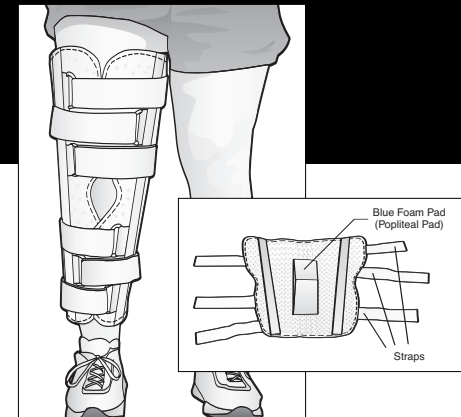

IMPORTANT INFORMATION

Please read carefully and completely before applying.

INTENDED USE

For immobilization of the knee joint, post-operatively or after joint injury.

INDICATIONS

Post-operative knee immobilization, Grade II or III ligament sprains.

CONTRAINDICATIONS

Patients with poor peripheral circulation, diabetes or decrease in skin sensitivity should not use a knee immobilizer.

PRECAUTIONS

- Consult your medical professional immediately if you experience sensation changes, unusual reactions, swelling or prolonged pain while using this product.
- The knee immobilizer should fit, generally, 2" above ankle bones and 2" below groin. Any longer could result in abnormal wear and skin pressure.

Sized Knee Immobilizer SIZING CHART






	Knee Circumference
S	14"-16"
M	16"-18"
L	18"-20"
XL	20"-22"
XXL	22"-24"
XXXL	24"-26"


INSTRUCTIONS FOR USE

- Place brace against the leg such that the metal stay runs down the back of the leg (anteriorly).
- If the blue foam popliteal pad is ordered by clinician, remove paper backing to expose adhesive and apply to the knee immobilizer as shown.
- Close the brace so that the patella notch surrounds the knee.
- Buckle the straps immediately below and above the knee joint. Buckle in an alternating below and above fashion until all of the straps are secure.
- Adjust all straps for a snug, yet comfortable fit.

CLEANING INSTRUCTIONS

Hand wash with mild detergent in lukewarm water.
Air dry.




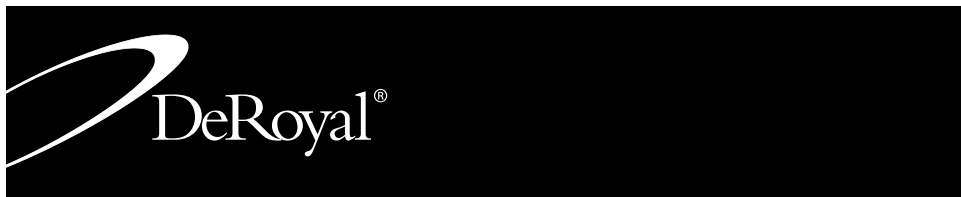


Tri-Panel Knee Immobilizer

INSTRUCTIONS FOR USE


1. Remove panels from center body.




2. Wrap center body around the leg.



3. Attach medial and lateral panels in desired position.




4. Buckle the straps immediately below and above the knee joint. Buckle in an alternating below and above fashion until all of the straps are secure.




5. Adjust all straps for a snug, yet comfortable fit.

3. Move medial and lateral stays into the desired medial and lateral position.



4. Buckle the straps immediately below and above the knee joint. Buckle in an alternating below and above fashion until all of the straps are secure.



5. Adjust all straps for a snug, yet comfortable fit.



Manufacturer

DeRoyal
200 DeBusk Lane, Powell, TN 37849 U.S.A.
888.938.7828
865.938.7828

Authorized Representative

DeRoyal Europe, Ltd.
Virginia Road, Kells, County Meath Ireland
353.46.9280100


Part #0-1430
Revised 5/07

©2007 DeRoyal. All Rights Reserved.


Universal Cutaway Knee Immobilizer

INSTRUCTIONS FOR USE


1. Place brace against the leg with the contoured metal stay running down the back of the leg contouring to the leg anatomy.



2. a) Close the garment around the leg.




b) If the immobilizer is too large, trim excess material for a more intimate fit.




Tri-Panel Knee Immobilizer

INSTRUCTIONS FOR USE


1. Remove panels from center body.




2. Wrap center body around the leg.



3. Attach medial and lateral panels in desired position.




4. Buckle the straps immediately below and above the knee joint. Buckle in an alternating below and above fashion until all of the straps are secure.




5. Adjust all straps for a snug, yet comfortable fit.

3. Move medial and lateral stays into the desired medial and lateral position.



4. Buckle the straps immediately below and above the knee joint. Buckle in an alternating below and above fashion until all of the straps are secure.



5. Adjust all straps for a snug, yet comfortable fit.



Manufacturer

DeRoyal
200 DeBusk Lane, Powell, TN 37849 U.S.A.
888.938.7828
865.938.7828

Authorized Representative

DeRoyal Europe, Ltd.
Virginia Road, Kells, County Meath Ireland
353.46.9280100


Part #0-1430
Revised 5/07

©2007 DeRoyal. All Rights Reserved.


Universal Cutaway Knee Immobilizer

INSTRUCTIONS FOR USE

1. Place brace against the leg with the contoured metal stay running down the back of the leg contouring to the leg anatomy.



2. a) Close the garment around the leg.



b) If the immobilizer is too large, trim excess material for a more intimate fit.

